



VISCOJECT-BIO 1.8 Injector Set

Handling instructions for
non-preloaded ZEISS MICS IOLs




We make it visible.

VISCOJECT-BIO 1.8 Injector Set

Preparing the non-preloaded ZEISS MICS IOLs for use




Place a small amount of OVD* in the cartridge tip. Place a line of OVD in each channel of the cartridge. Do not touch the tip of the cartridge.

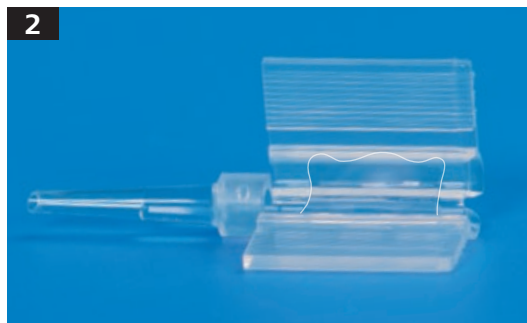

Place the lens in the center of the open cartridge. Push down on the edges of the optic to ensure that the optic haptics are positioned under the ledges of the cartridge.



For toric and multifocal IOLs, mind the orientation holes and the meridian marks.

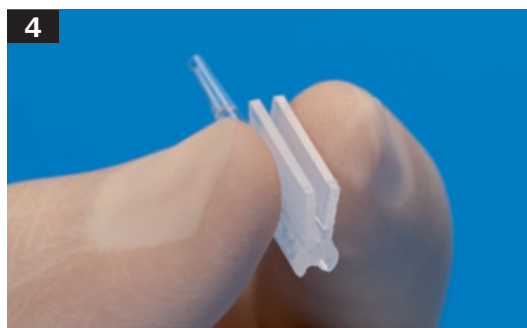

Maintain the IOL in place with the folding forceps while folding the cartridge. Close the cartridge until you hear a click.



Place the cartridge into the injector and move it forward as far as it will go. The lens is ready for implantation.



Place the bevelled edge downward and gently push the plunger to inject the IOL.

*Carl Zeiss Meditec recommends the use of ZEISS OVDs.

EN_32_022_00131
VISCOJECT is a trademark of Meditel (CE 0482). The contents of the brochure may differ from the current status of approval of the product in your country. Please contact our regional representative for more information. Subject to change in design and scope of delivery and as a result of ongoing technical development. Printed on elemental chlorine-free bleached paper.
© 2015 by Carl Zeiss Meditec AG. All copyrights reserved.



Carl Zeiss Meditec AG
Goeschwitzer Str. 51–52
07745 Jena
Germany
www.meditec.zeiss.com/iol
www.meditec.zeiss.com/contacts